

Delayed

20 May 20 10:55:30 HR 100  
Manual Lead II 10mm/mV 1-30 Hz



Print Strip

PHILIP

Delayed

20 May 20 11:01:15 HR 127  
Manual Lead II 10mm/mV 1-30 Hz



PHILIP Print Strip

PHILIP


LONG LEADS AND DEEP INSPIRATION (DI)

CARDIART

Убайдулла

20/11/2020 1:30 PM

10mm/IV 2.5mm/50 25 35Hz

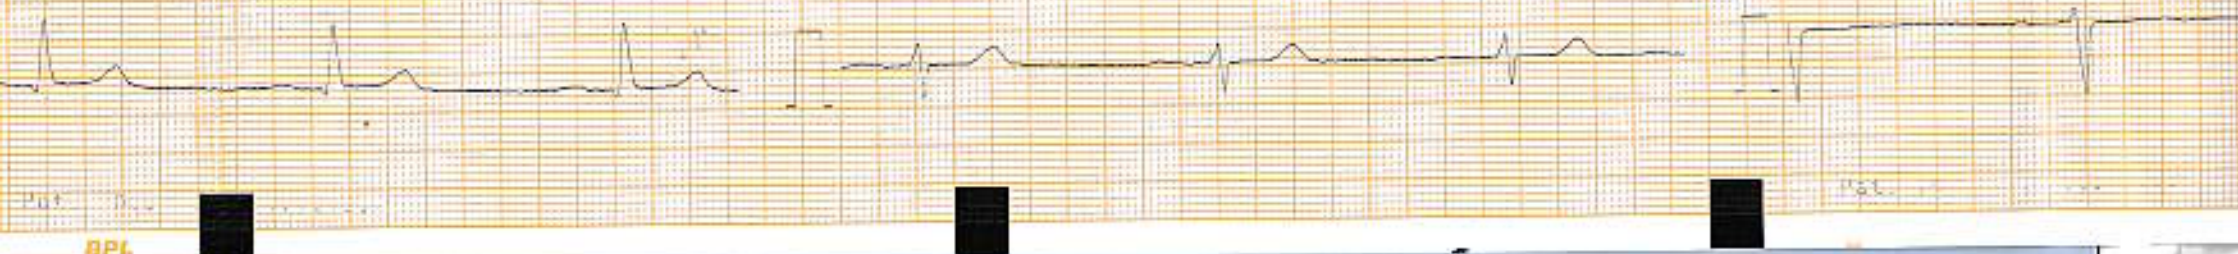

BPL

CARDIART

BPL CARDIART 6198T




10mm/IV 2.5mm/50 25 35Hz

BPL LA 350M



BPL

LONG LEADS AND DEEP INSPIRATION (DI)

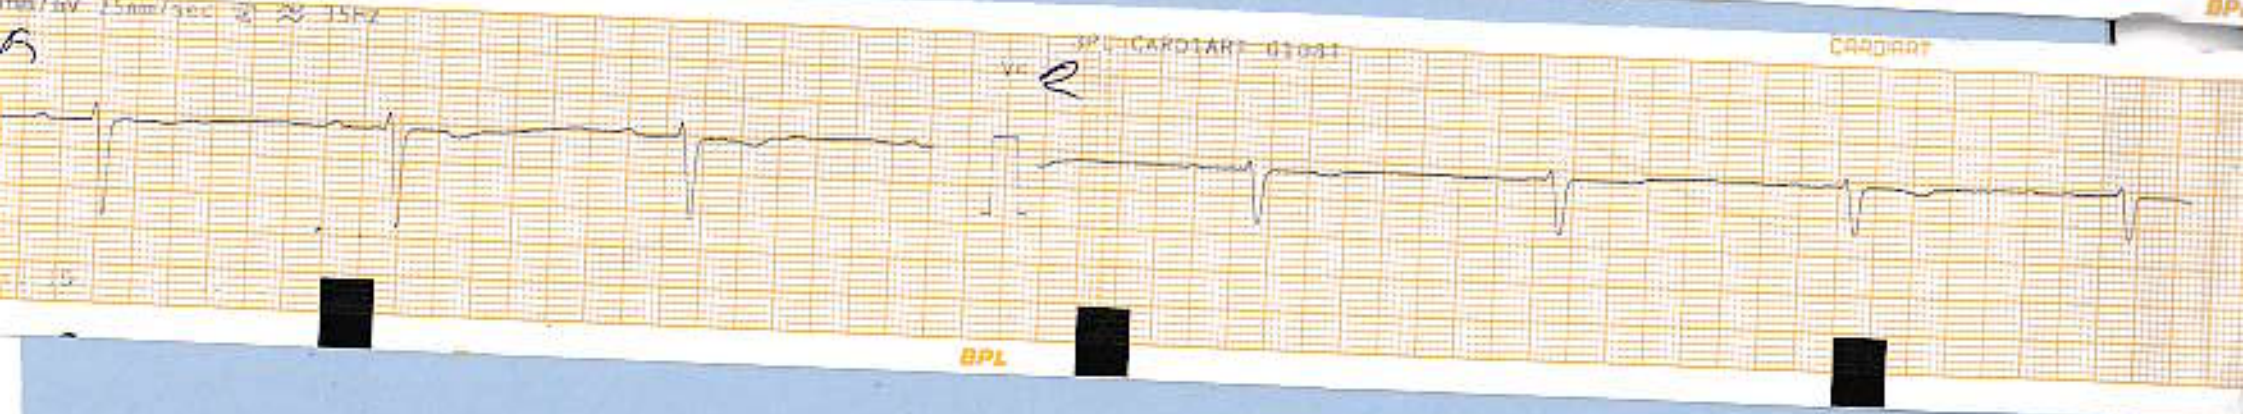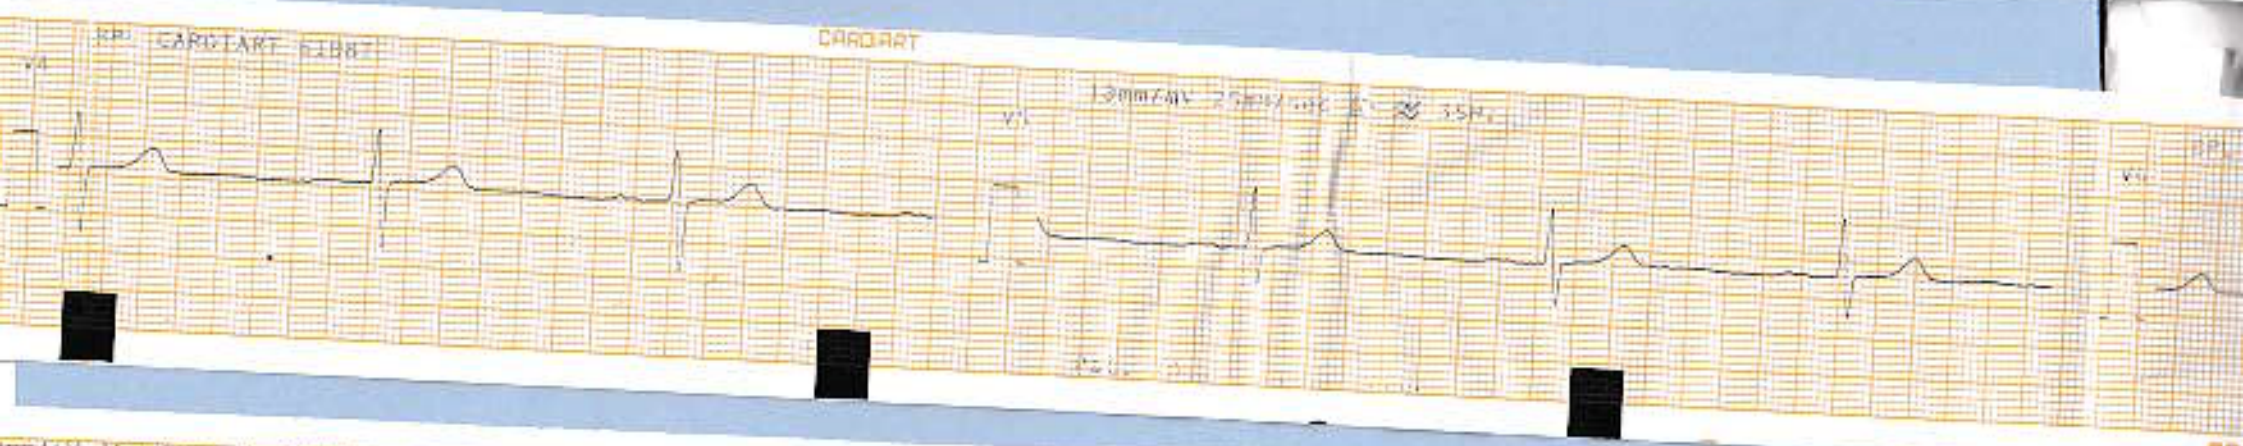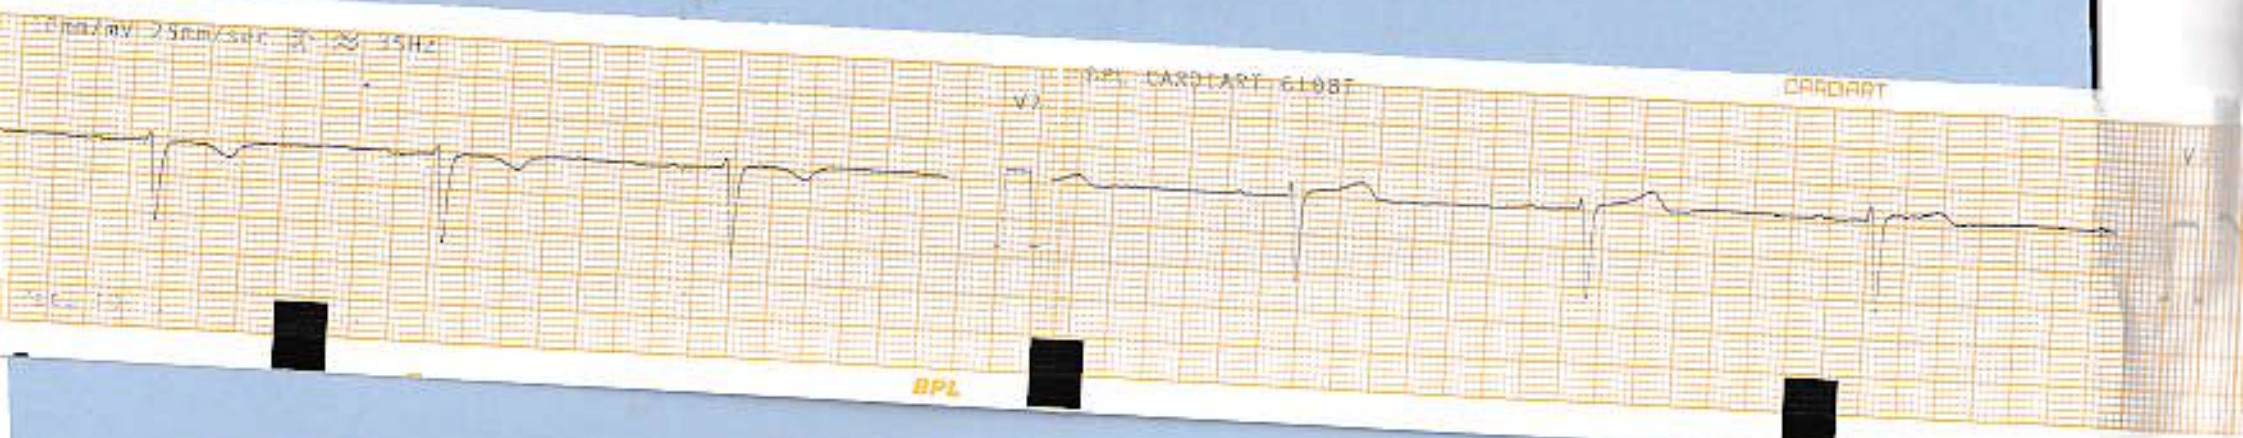

20-May-2020 11:26:53


PRINTED IN USA

GE Healthcare

REF: 2164773001

CE

PRINTED IN USA



Name/ID: .....

Vent. rate 133 bpm  
 QRS duration 102 ms  
 QT/QTc 316/470 ms  
 PR interval \* ms  
 P duration 0 ms  
 RR interval 451 ms  
 P-R-T axes + -38 134

MACi V2.00

12SL v239

Supraventricular tachycardia  
 Left axis deviation  
 ST & T wave abnormality, consider  
 lateral ischemia  
 Abnormal ECG

GE 20-May-2020 11:27:43

PRINTED IN USA

GE Healthcare

REF: 2164773001

CE

MACi V2.00

Name/ID: .....



MACi V2.00

12SL v239

50Hz



Continuous rhythm

0.16-20Hz

25.0 mm/s

10.0 mm/mV

STD

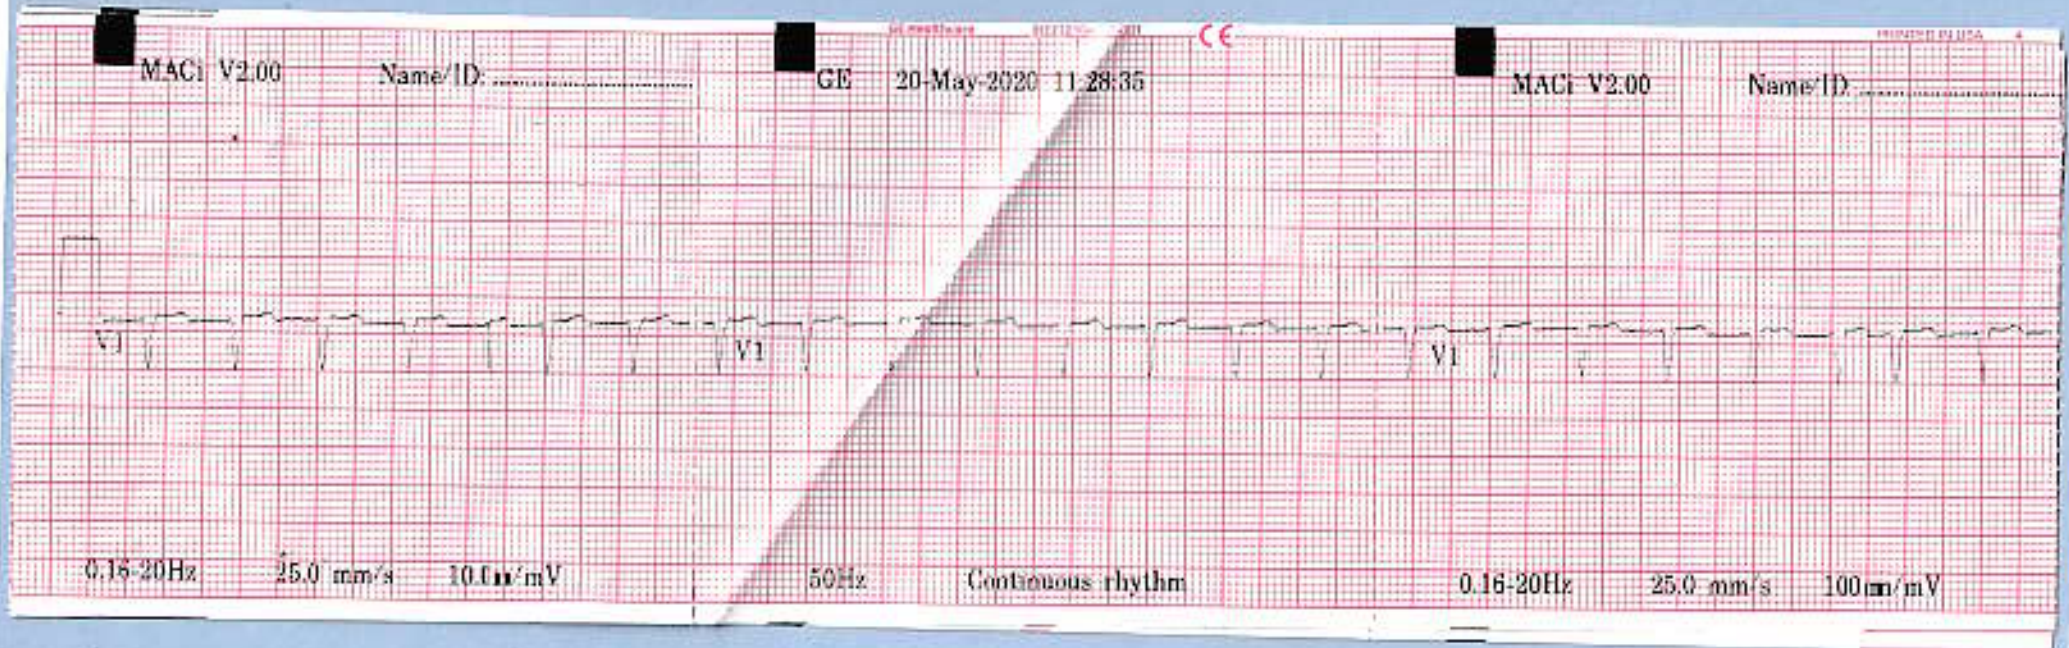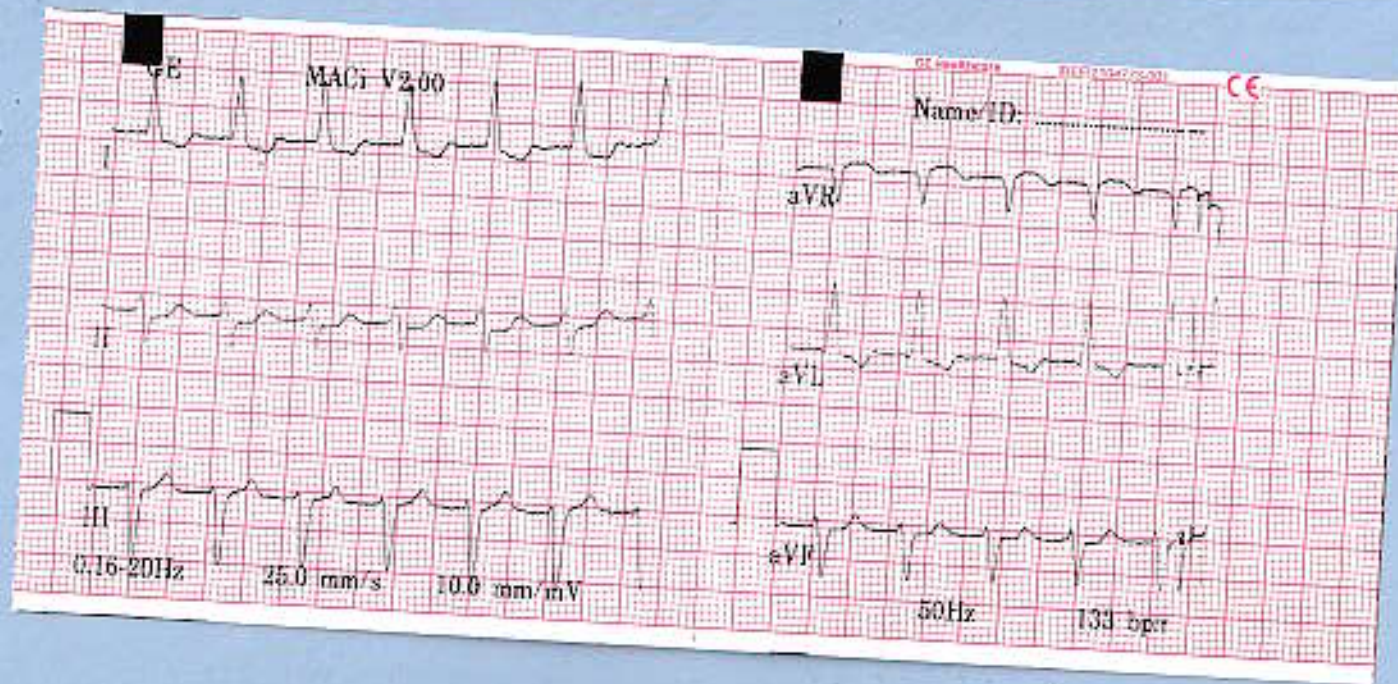

ECG

Mrs. Hafuniza Goyx/Re 210510000 at  
5 cm

BPL CARDIAC 61033

DATE/TIME 21/05/2024 10:25




BPL

CARDIAC 61033

20mm/10V 25mm/sec 21 22 23 24

CARDIAC

BPL

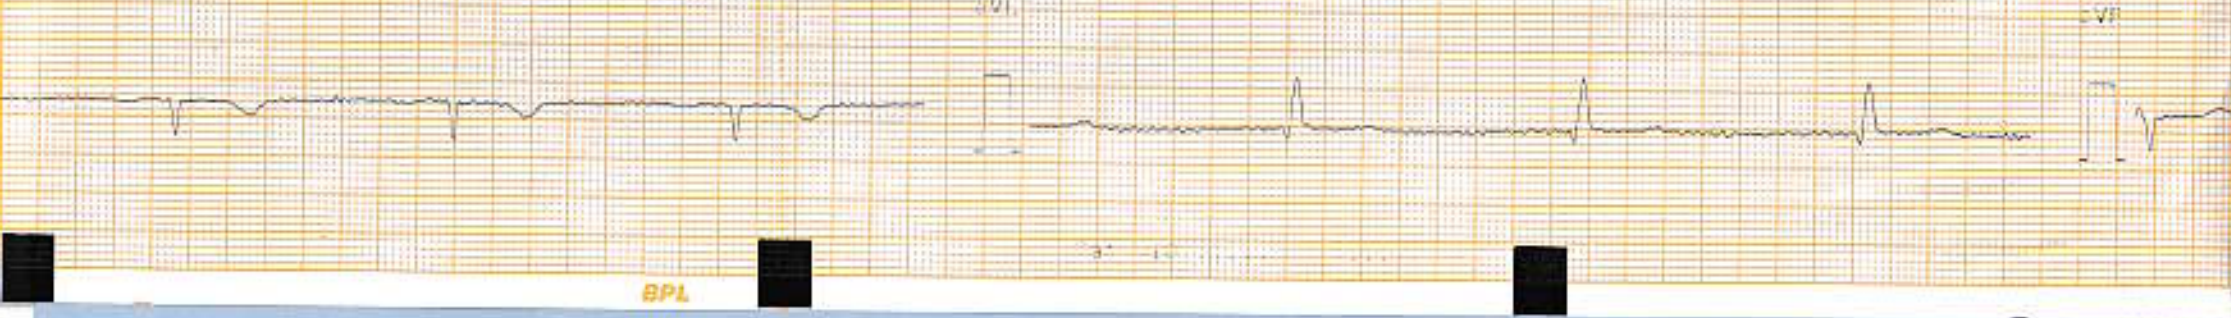

BPL

LONG LEADS AND DEEP INSPIRATION (DI)

