


STD

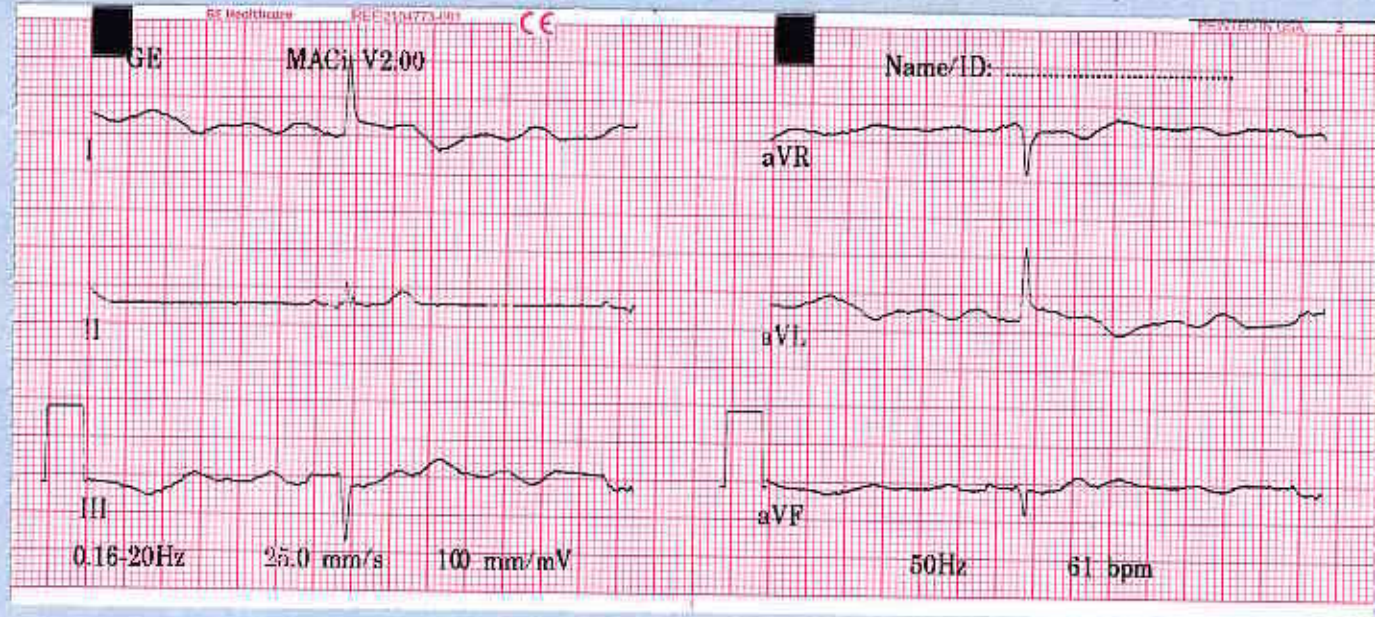


GE 9-Feb-2020 18:23:42

MACi V2.00

Name/ID: _____

GE 9-Feb-2020 18:23:57

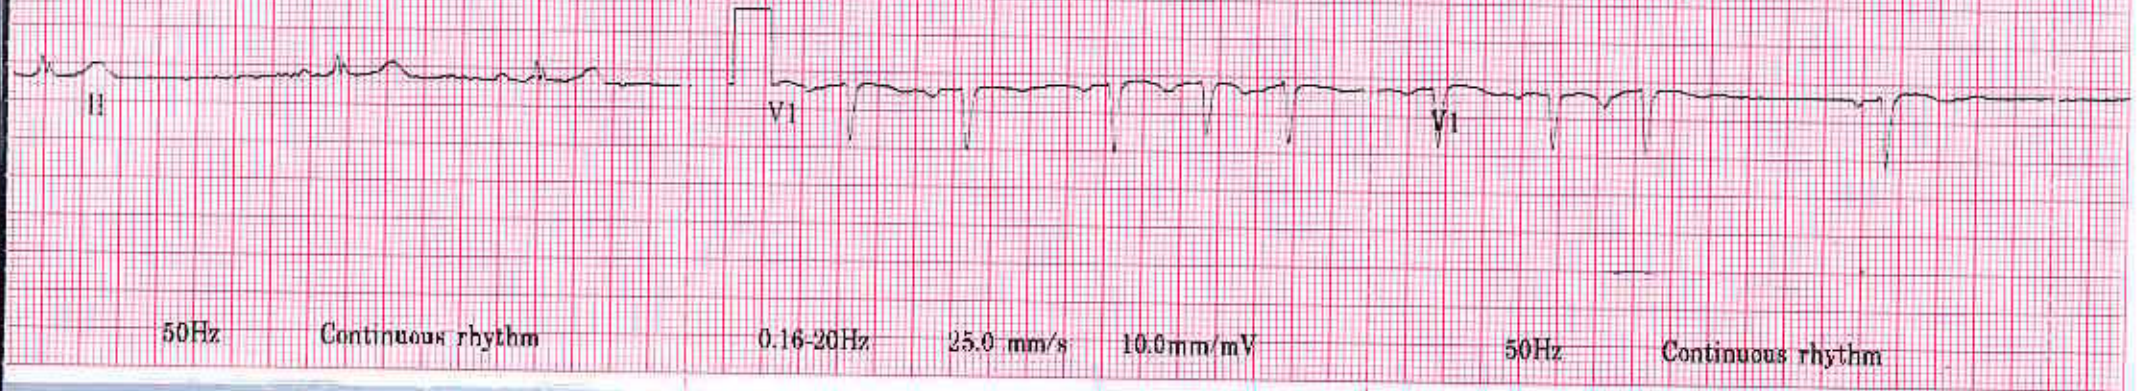

9-Feb-2020 18:22:50

GE Healthcare P11 20022400 CE

PRINTED IN USA

Name/ID:

V1

V4

V2

V5

V3

V6

Simultaneous-3

Vent. rate	61 bpm
QRS duration	92 ms
QT/QTc	430/432 ms
PR interval	* ms
P duration	0 ms
RR interval	983 ms
P-R-T axes	* -17 -7

MACi V2.00

12SL™ v239

9/2/2020

GE Healthcare P11 2104773-001 CE

MACi V2.00

Name/ID:

Atrial fibrillation
Abnormal ECG

V4

MACi V2.00

Name/ID:

V3

MACi V2.00

12SL™ v239

0.16-20Hz

25.0 mm/s

10.0 mm/mV

0.16-20Hz

25.0 mm/s

10.0 mm/mV