

GE Healthcare

10-Apr-2021 4:41:19

REF I019778LSI CE LOT D653

Name/ID:

V1

V4

V2

V5

V3

V6

Simultaneous-3

Vent. rate	84 bpm
QRS duration	192 ms
QT/QTc	494/583 ms
PR interval	* ms
P duration	0 ms
RR interval	714 ms
P-R-T axes	* -68 7

MACi V2.00

12SL™ v239

GE Healthcare

REF I019778LSI CE LOT D653

MACi V2.00

Name/ID:

MACi V2.00

Name/ID:

Atrial fibrillation with a competing junctional pacemaker
 Right bundle branch block
 Left anterior fascicular block
 *** Bifascicular block ***
 T wave abnormality, consider lateral ischemia or digitalis effect
 Abnormal ECG

(P)

(P)

V3

V4

MACi V2.00

12SL™ v239

0.16-40Hz

25.0 mm/s


10.0 mm/mV

0.16-40Hz

25.0 mm/s

10.0 mm/mV

STD

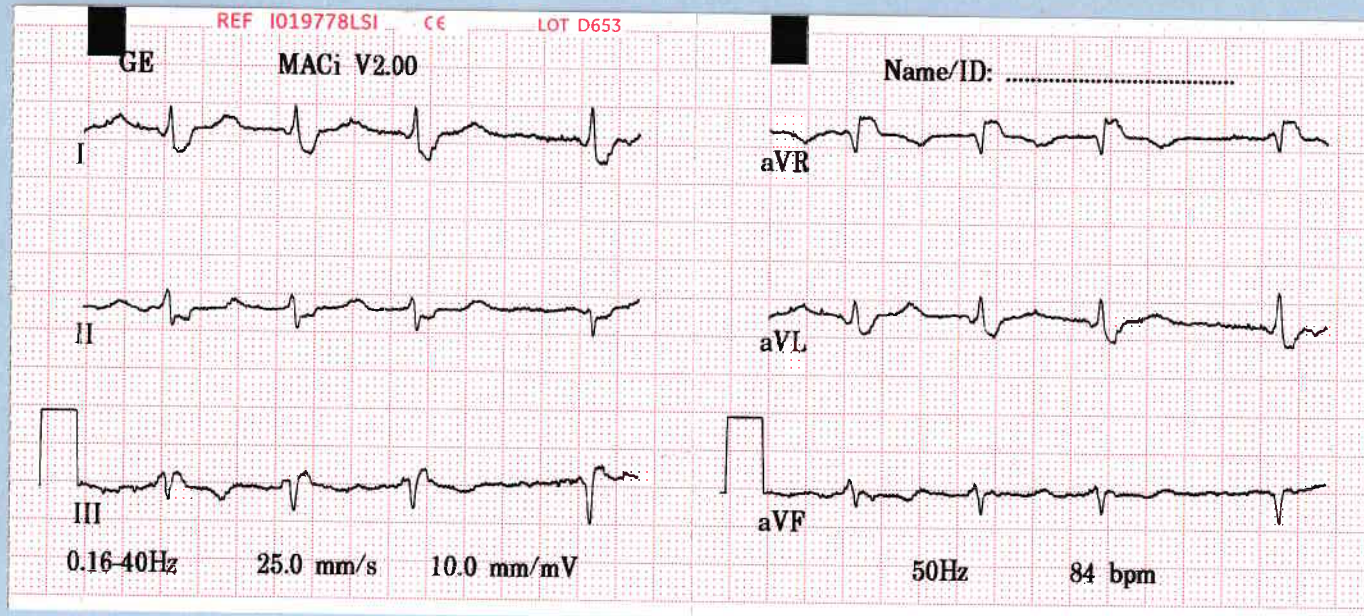

LONG LEADS AND DEEP INSPIRATION (DI)